



Bioabsorbable Screws for Anterior Cruciate Ligament Reconstruction Surgery: A Review

J. Esmailzadeh^{a*}, H. Setayesh^b

^a Department of Material and Chemical Engineering, Esfarayen University of Technology, Esfarayen, North Khorasan, Iran

^b Department of Materials and Metallurgical Engineering, Faculty of Engineering, Ferdowsi University of Mashhad, Mashhad, Razavi Khorasan, Iran

PAPER INFO

Paper History:

Received 17 April 2020
Accepted in revised form 08 July 2020

Keywords:

Anterior Cruciate Ligament
Reconstruction
Bioabsorbable Screws Mechanical
Properties
Biological Properties

ABSTRACT

One of the popular orthopedic implants is utilizing fixation screws to fix Anterior Cruciate Ligament (ACL) grafts and secure the graft into femur and tibia. Currently, these screws are made of titanium or bioabsorbable materials. In this respect, bioabsorbable screws were generated in order to overcome some of the potential problems caused by metallic screws. Although the bioabsorbable screws are susceptible to some drawbacks including bone ingrowth features as well as good in vitro and in vivo mechanical properties. The biomechanical results of ACL screws showed that the ultimate failure loads and yield point loads varied from 800-1500 N and 600-1000 N, respectively. Moreover, the evaluations of in vivo degradation behavior showed the almost complete or fully complete resorption of ACL screws from 6 month to 2 years. However, it was proved that the addition of bone mineral phases such as Hydroxyapatite (HA), β -Tricalcium Phosphate (β -TCP), and Calcium Carbonate (CC) could enhance this degradation rate. Incorporation of biceramics into pure polymeric ACL screws may contribute to enhancing the osteogenesis of bone after full resorption of screws, function as buffering agents that decrease the acidity of screw adjacents resulting from degradation of products, and improve the mechanical properties of ACL screws. In this paper, the latest bioabsorbable ACL screws which are currently available for graft fixation in orthopedic markets are discussed. A brief review of the literature regarding the physical, biological, and mechanical properties of bioabsorbable ACL screws was made. Besides, the insertion technique, various manufactured sizes, and in vitro and in vivo mechanical properties for each screw were addressed.

1. INTRODUCTION

In orthopedic surgery, biomaterials such as metals, ceramics, polymers, and composites are used as implants which are well compatible with living body tissues [1]. For many years, various metal alloys have been extensively used to fix the fractured bone or soft tissue rupture due to their desired mechanical properties and at the same time, their own proper biocompatibility [2]. Common orthopedic alloys are stainless steel, cobalt-chrome, titanium, and magnesium alloys [3]. Bone is a dynamic and complex live tissue that provides the body with the required mechanical endurance and has an elastic modulus of 10 to 30 GPa [4]. Among all of orthopedic devices used for fixation and preservation of damaged bone or soft tissues in order to restore their functions, Anterior Cruciate Ligament Reconstruction (ACLR) screws are one of the most popular orthopedic devices. The stability of knee joint is provided by four

extremely strong ligaments: ACL and Posterior Cruciate Ligament (PCL) prevent the tibia from slipping in sagittal planes; Medial Collateral Ligament (MCL) and Lateral Collateral Ligament (LCL) prevent the knee from bending in coronal plan. Among them, ACL tearing is one of the most common injuries (11 to 33% in different series) which is prevalent among athletes or patients with high activity. Fixing the graft into bone tunnel is a substantial step during the ACL reconstruction surgery. In this regard, the graft is threaded and compressed into bone pilot drilled hole by interference screws. There are two different types of ACL screws: metallic and degradable polymer-based screws. Use of metallic screws are regarded as the standard graft fixation method [5, 6]. The first ACL interference screws made of titanium alloys with a relatively sharp thread were utilized to provide a good anchorage of BPTB grafts into bone tunnel [7].

* Corresponding Author Email: Esmailzadehj@esfarayen.ac.ir (J. Esmailzadeh)

Such screws were first introduced by Lambert [8] in 1983 and then, popularized by Kurosaka et al. [9]. However, titanium screws provide high initial strength and well integration into the adjacent bone due to good biocompatibility; in some cases which need to be revised, the screw removal is known as a challenging issue [10,11]. The advantages of metallic ACL screws are solid fixation and well toleration on behalf of the body, while some of their drawbacks are their interferences with any applied probable Magnetic Resonance Imaging (MRI) following the surgery [1] and their potential interferences with any future surgeries on the knee such as ACL reconstruction, which may cause the laceration of the graft during insertion [12,13]. Currently, many attempts have been made to replace the retained unneeded foreign body materials into body by biodegradable and bioabsorbable ones. Bioabsorbable ACL screws could disappear when they are no longer needed. These categories of ACL screws are capable of overcoming some of the potential problems prevalent in metallic ACL screws. However, bioabsorbable ACL screws have their drawbacks including their fragility during insertion or inflammatory reactions [7]. Therefore, preserving the mechanical and biological properties of materials during the graft healing process is a crucial challenge. Bioabsorbable interference screws were first introduced for arthroscopic ACL reconstruction applications in the early 1990s [14]. More recent interference screws are made of biodegradable polymers or polymer/ceramic composites [2]. Different combinations of synthetic materials used as the major components of biodegradable ACL screws are Polylactic Acid (PLA) and its various enantiomers, Poly-L-lactic Acid and Poly-D-lactic Acid, Polyglycolic Acid (PGA), and copolymers of PGA/PLA. While PLA, the mainly used material, is characterized by a longer resorption time (yearly basis), the resorption takes a shorter amount of time for the PGA and PGA/PLA copolymers (monthly basis). Currently, various commercial ACLR screws are characterized by different mechanical and biological properties owing to their different chemical composition contents. These screws are usually fabricated by several companies. While substantial biodegradable polymeric ACL reconstruction screws are commonly made of biodegradable polymeric components such as PLA and its enantiomers, PGA, PLC, and some other screws have a bioceramic osteoconductive and osteoinductive fillers such as HA, BCP, TMC, β -TCP, and bioactive glass. Table 1 presents a list of some of these screws containing different polymers and copolymers formulation and those containing osteoinductive and osteoconductive filler phase. The present study aims to present a whole series of commercial ACLR screws regarding their material compositions, in vitro and in vivo studies, biodegradation behavior, and mechanical and physical properties. The hypothesis here suggests

that this collection can promote scientific research since such an issue has not been previously elaborated in the literature.

2. ANTERIOR CRUCIATE LIGAMENT RECONSTRUCTION SCREWS

In orthopedic surgery, ACLR is performed by interference screws to maintain ligament inside the bone until the tissue is remodeled. These screws are fixed into a space between the bone plugs and drilled tunnel walls. These kinds of screws are available in different sizes to meet the patient's requirements. To ensure that the screws are implanted at the appropriate angle and direction, a wire with a proper diameter is used is drawn from the inside of the screw and drill hole (Figure 1) [15]. Currently, several companies manufacture reconstruction screws used in ACL surgeries. While most commercial screws have a similar hollow socket to drive the screws, significant differences in their designs make the distinctions between different companies. For example, some parameters that usually differentiate a company's products are the diameter or length size, screw tapering, threads geometry, thread pitch, and material type. The materials used to make the screws is among those criteria that make the difference. Conventional reconstruction screws are usually made of Titanium due to its biocompatibility and acceptable mechanical and physical features; however, in the past decade, other compounds were also developed. New screws are mainly characterized by their absorbable materials in compositions that are degraded into the body, while the metal ones will remain permanently within the bone [16]. However, the probability of inherent problems caused by the absorbable interference screws for ligaments and tendon reconstructions has not been entirely proven yet.

It should be noted that a harmonic trend of the mechanical properties of loosening due to degradation of screw constructs and tendon healing process is a significant issue. Therefore, if the metal screws are replaced by biodegradable ones, it must show adequate fixation for at least 6–8 weeks until the bone block has been incorporated and biological fixation has been achieved [17,18]. It can be found that the almost whole bioscrews composed of synthetic polymers such as PLA, PGA, etc. have acid-based ingredients. While these screws that are exposed to aqueous medium into the body and reabsorbed by hydrolysis and their products dissolve in water forming liquid acids. In a specific area with good blood supply within the body, the acid is well buffered and metabolized; however, in areas with poor blood supply such as bone, the pH of the screw-adjacent medium can be quite low. A decrease in pH of the adjacent tissue results in an

accelerating rate of screw degradation, tissue damaging, and bone destruction.

This is the reason why manufacturers, in some cases of ACL screws, have added bioceramics such as hydroxyapatite and tri-calcium phosphate into the material formulations. These materials could promote the osteoconduction and osteinduction characteristics of screws and neutralize the screw-adjacent acidic medium caused by acidic products of screw degradation resulting from the alkaline ions release.

In addition to screw formulation, various other parameters including component composition, size of acidic crystals, screw geometry, and manufacturing method were identified that would influence the behaviors of screws in implant sites. Thus, all bioscrews are not equal and do not behave the same, even if they have been made from the same materials at different implants [19].

TABLE 1. Current commercial Bioabsorbable screws

Manufacturer	Composition	Bioabsorbable Screws
Inion Ltd.	PDLLA/Tri-methylenecarbonate (TMC)	Inion Hexalon
Smith &Nephew	PGA/Tri-methylenecarbonate (TMC)	EndoFix
	PGA-co-PDLLA/Calciumcarbonate (CC)	Calaxo
DePuyMitek, Inc.	PLLA/ β -Tricalciumphosphate (β -TCP)	Bio-IntrafixBiocryl
ArthroCare Corporation		Bilok
DePuyMitek, Inc.	PLGA/ β -Tricalciumphosphate (β -TCP)	Milagro
ConmedLintratec	PDLLA/ β -Tricalciumphosphate (β -TCP)	Osteo ACL Screw
	SR-PDLLA/ β -Tricalciumphosphate (β -TCP)	Matryx
Smith &Nephew	PLLA/Hydroxyapatite	Biorci-HA
Stryker		Biosteon
Arthrex, Inc.	PDLLA/Biphasic calciumphosphate (BCP)	BioComposite
ConmedLintratec	SR-PDLLA	SmartScrew
Bioscience, Ltd.	SR-PLLA	Biofix
CenterpulseMedicalAG	PDLLA	Sysorb
Biomet SportsMedicine, Inc.	PLLA-co-PGA	GentleThreadsBioCore
Karl Storz-EndoscopePhusis	PLLA-co-PDLLA	MegaFixPhusiline
Instrument Makar, Inc.	PGA-co-PDLLA	Biologically Quiet
Arthrex, Inc.	PLLA	Delta Tapered Bio-interference Screw
		Round Delta Tapered Bio-interference Screw
		Bio-interference Screw
		Biocortical Screw
		RetroScrew
		Full Thread

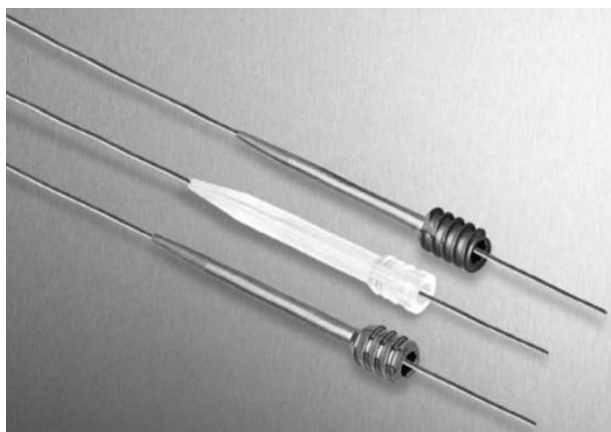


Figure 1. Example of guide wire of ACL reconstruction screws [15]

Of note, it has been reported that the tunnel widening for a poly-levodextro-lactide (PLDLA) and β -tricalcium phosphate composite screw did not occur [20], while this is a common occurrence for other series [21,22].

A study on a comparison of different combinations of absorbable interference screws showed that Poly L-Lactide (PLLA) was not completely degraded after 20 months of implantation. However, poly(DL-Lactide-co-glycolide) (PDLA-co-PGA) undergoes complete degradation during this period of time. Although no damage has been reported for poly(DL-Lactide-Acid) (PDLA) up to 6 weeks, it would be completely degraded within 10 months [23]. The degradation rate of ACL screws should be in agreement with the biological tissue growth. Bach et al. [24] evaluated the tissue growth surrounding the surgical site in ACLR with the screws made of 32.5% tri-methylene carbonate and 67.5% polyglycolide. This study conducted experiments on 20, 10, and 8 patients over 6, 12, and 24 months, respectively. The clinical and MR imaging results indicated that according to Figure 2(a-b), the screws were partially resorbed within 6 months and completely resorbed within 12 months; besides, according to Figure 2(c), these screws enlarged the bone tunnel as a result of screw replacement [24]. Another potential problem of absorbable interference screws is caused by their degradation. As the biodegradable screws breakdown, their molecules and components will be released, causing inflammatory reactions through the foreign body responses. These reactions may be either minor, releasing a small non-bacterial sinus, or significant which requires immediate attention. Although screws with long degradation time duration will cause fewer foreign body reactions, they will simultaneously require a longer period of time to complete the bone regeneration. However, it was observed in most cases that the body did not completely repel the screw until the emergence of foreign body reactions, hence the cysts formation and osteolysis [25].

Moreover, as reported in several studies, late inflammatory reactions appeared after ACL surgery. Morgan et al. [26] elaborated on the advantages of explants made of screw remnants, fibrous connective tissue, cortical-like bone, and cancellous bone due to PLLA interference screws after 30 months. Similarly, Park and Tibone [27] observed the persistence of tibial PLA interference screws 4 years past the ACL surgery, which was approved by MRI. However, under irrigation, no screw was found, probably due to late inflammatory reaction.

However, the new bone formation through replacement of ACL screws is only observed for bioscrews independent of its formulation with a slow rate of degradation manner in excess of 5 years [19, 28].

Several studies compared the biodegradable and metallic screws and suggested that bioabsorbable screws would provide good fixation like metal screws; therefore, these screws could be a rational alternative to metallic ones [29-35].

For example, on the comparison of bioabsorbable and metallic ACL reconstruction screws for graft fixation, a number of researchers have found no significant difference in the final patient outcomes in terms of clinical scores, clinical evaluation, and imaging assessments [32]. Moreover, in terms of the range of motions, the obtained comparative results of bioabsorbable and metallic screws for different fixations of grafts confirmed that there was no significant difference between the two groups in the long term, as seen in studies [29,33,36]. Concerning the functional outcomes, Rocco Papalia et al. [37] found no differences between the two types of screws.

3. ACL RECONSTRUCTION SURGERY

ACL injuries are very common, with around more than 4 million reconstruction and healing surgery every year all over the world [38]. This type of injury may occur due to severe knee blowing, sudden stopping, sudden turning, or severe stretching. Individuals who play sports like skiing, football, and basketball are more prone to ACL ligament injury than any other groups [39]. When an ACL injury occurs, the injured usually hear a pop sound, followed by a mild pain that causes swelling in the affected area [15]. The diagnosis of quick ACL tearing is performed by asking the patient to relax his/her legs and the doctor pulls the patient's legs forward to see if the bone is limited to moving in the anterior direction or not; this test is called the Lachman displacement test [15]. Now, if the bone has no limitation in displacement, it can be concluded that the ligament is torn. In this case, MRI can easily determine the ACL rupture. Reconstruction of the ACL involves the replacement of the old ligament by a tissue graft and is usually harvested from the hamstring tendon or

patellar tendon [15]. Harvesting of the graft is the first part of the ACL surgery. In the case of patellar, the surgeon creates an incision on the patellar which is of less importance. In the following, the central part, the attached and cylindrical portions of the tendon are removed outside the femoral and tibia head, so-called bone plugs. The end of the remaining tendon is sutured to regrow and continue to perform its duties. After the graft harvesting, sutures are added to the bone part of graft used in placing the tendon. Then, the remains of ACL are removed from the knee and pierces of the inter condylar notch burred away so that the surgeon will have a chance to reach the correct placement of the tendon. To complete the perforation, the surgeon creates two holes in the upper part of tibia and the lower part of the femur near the knee (Figure 3) [15]. To create each of these holes, a small hole is initially created by a small diameter drill to increase the accuracy of perforation and then, by a drill with a diameter similar to the cylindrical bone plug. After the holes are smoothed, the sutured end of the graft is inserted to the knee through tibia head, while the other end is pulled out from the femoral head [15]. The graft is tightened using the interference screws. The biodegradable interference screws keep the tendon firm within the bone (Figure. 4) [15]. After the surgery, the patient will have a fairly moderate pain and difficulty bending and extending the knee. In addition, postoperative activities are limited and a hard rehab program must be tolerated to be restored. Since the graft is gradually becoming a tendon, the postoperative activities should be limited to be well applied. During this process, the graft is very weak and the knee is partially unstable. The emergence of a tear is possible in case such activities are intense and uncontrolled. Setting a limit on these activities is absolutely necessary because the graft is only kept by an interference screw. Therefore, as the graft is being pulled by the tibia and femoral bone, the screw will be pulled out of the hole. This scenario may also lead to another reconstruction.

4. BIOABSORBABLE POLYMERIC ACL SCREWS

4.1. PLLA-BASED ACL SCREWS

Among the biopolymers that belong to poly (α -hydroxy acids) family, PLA is extremely well known and widely studied. PLLA is a kind of PLA enantiomer that is a common biodegradable polymer used in the compositions of ACL fixation screws. They go through a degradation process mainly due to the hydrolysis mechanism. Throughout the degradation, water diffuses into the structure which leads to a break in the long chains and changes them to small oligomers that can diffuse inside and outside of the polymeric matrix. These degradation products can be eliminated from the

human's body through the Krebs cycle (using urination or CO₂ gas during breathing) [40].

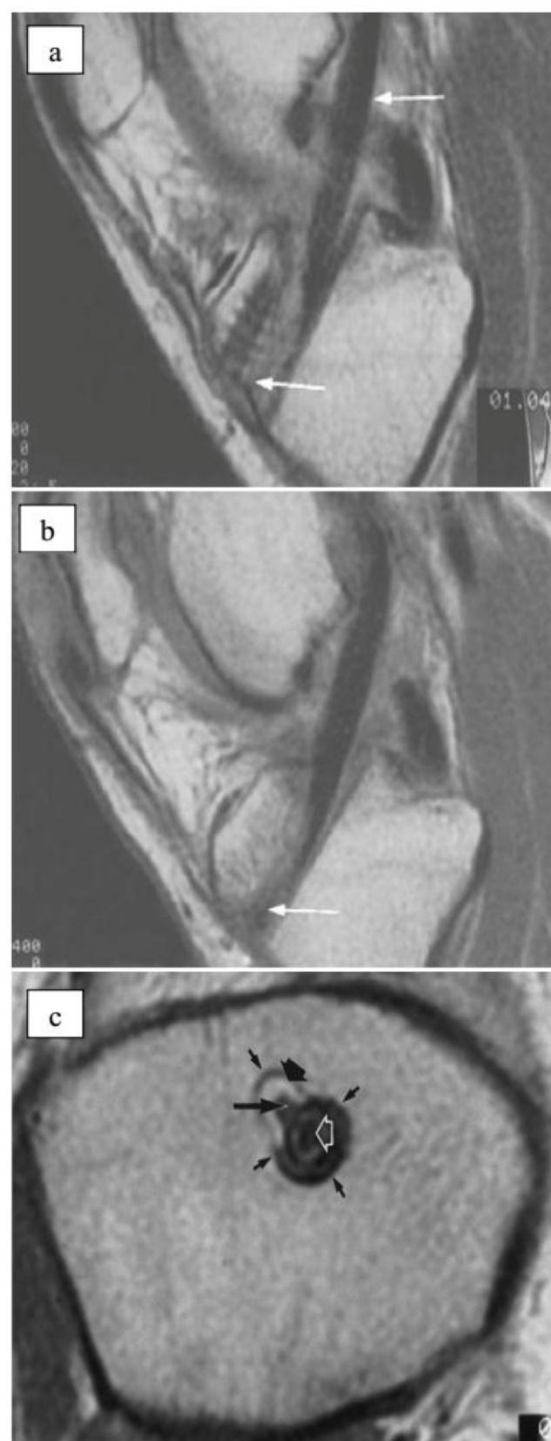


Figure 2. a) Magnetic Resonance Images (MRI) of partial resorption of interference ACL screws at 6 month following implantation, b) total resorption at 12 month following implantation, and c) implantation tunnel after total resorption. New tissue formed around the bone plug (open arrow) determined fibrous tissue (long skinny arrow) with fatty tissue surrounding it (thick short solid arrow) [24]

PLLA molecular weight varies due to its manufacturing technique; for instance, PLLA with high molecular weight (>100 kDa) has a melting point around 137 °C to 178 °C and T_g temperature of 58 °C. Although PLLA is totally semicrystalline, its injection molding also makes nanocrystalline products, leading to a biomaterial whose modulus drops above the glass transition temperature [41]. In order to enhance the PLLA mechanical properties, an alternative strategy called self-reinforced polymer composites can be implemented. The fiber reinforcement in these materials is a highly orientated version of the same polymer from which the matrix is made [42]. For example, a PLLA matrix is reinforced with highly orientated PLA fibers.

Several studies reported the in-vitro results of PLLA-based screw degradation rate as well as body responses. In most of these screws, foreign body reaction during 20 to 30 months after the implantation indicated little or no evidence of inflammatory reaction within the implant environs. In some cases, body responses to screws offer little evidence of adverse inflammatory reaction which is related to the degradation of cartilage or loosening of knee joint envious especially in cases with retardation of screw degradation. Fixation strength of a biodegradable PLLA interference screw (Arthrex, Naples, FL) was compared with press-fit fixation and a titanium interference screw in ACLR using a Bone-Patellar Tendon-Bone (BPTB) graft. The results showed that there was no significant difference between the ultimate failure load of PLLA (805.2 N; range 680 to 995 N) and titanium interference screws (768.6 N; range 544 to 1094 N) [43]. The mechanical behavior of delta tapered bio-interference screws (PLLA nanocrystalline, Arthrex) as quadriceps hamstring tendon fixator was dynamically tested. It was found that the ultimate failure load and displacement at the break point of screws were 647 ± 200 and 10.91 ± 4.4 mm, respectively. The screws obtained their toughness of 64.54 ± 22.1 N/mm [44]. The biomechanical properties of Retro screws (Arthrex, PLLA) for tibial called anterior graft-tibial tunnel fixation were also obtained. The Retro screw displays superior toughness (114.1 ± 23.3 N/mm) and displacement (18 ± 0.5 mm) during cyclic testing. During load-failure testing, the maximum load of Retro screw failure was 787 ± 177.5 N. The displacement and toughness of bioscrew resulting from the pull-out test were 5.3 ± 2 mm and 204.4 ± 52.9 N/mm, respectively [45]. In another study on BPTB fixation Bioscrews (PLLA, Conmed Linvatec, Largo, FL) implanted into a cadaver, the results illustrated that the mean load to failure was 189 ± 118 N [46]. The fixation strength of BioFix screws (Self-reinforced (SR)-PLLA, Bio Science, Ltd, Tempere, Finland) in a BPTB graft within the bovine knee is 1211 ± 362 N and its elastic moduli in upper (>500 N) and lower (<500 N) range loads are 304 ± 71.8 N and 189 ± 47.4 N, respectively [47]. There is no significant difference between these biodegradable

screws and metal screws in the BPTB graft fixation in the bovine knee; therefore, they can be recommended regarding ACL reconstruction using this type of graft.

The mechanical properties of BIORCI screws (PLLA, Smith & Nephew, Andover, MA) for hybrid femoral fixation were investigated. The Ultimate Tensile Strength (UTS) of these screws was 643.5 ± 148.4 N and their toughness was reported as 315.7 ± 38.9 N/mm [48]. The initial fixation strength of two types of biodegradable screws consisted of Poly-L-Lactide/Tri-Calcium Phosphate (PLLA/TCP); one suspension screw (Bilok ST) with a diameter of 9 mm and length of 35 mm and the other interference screw (Bilok TS) with a diameter of 9 mm and length of 30 mm, determined in the hamstring reconstruction of ACL using bovine knees. The single-cycle test results showed that the maximum failure load, yield load, and stiffness were $1475.8 (\pm 315.3)$ N, $998.5 (\pm 122.56)$ N, and $248.1 (\pm 76.1)$ N/mm, respectively, in suspension screws group. For interference screws, the maximum failure load, yield load, and stiffness were measured $651.1 (\pm 155.4)$ N, $537.8 (\pm 86.7)$ N, and $199.5 (\pm 82.9)$ N/mm, respectively [49].

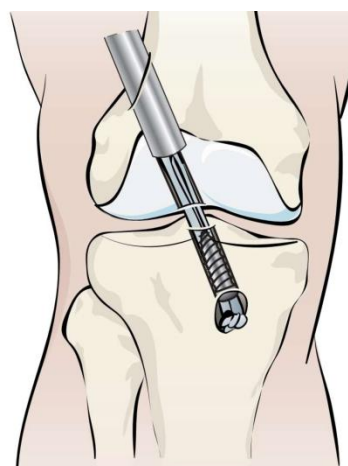


Figure 3. Creation of implantation holes at tibia and femur [15]

4.2. PDLLA-BASED ACL SCREWS

PDLLA is a copolymerization product of PLLA and PDLA as two enantiomers of PLA. Different mechanical properties of PDLLA are related to the composition percentage of each enantiomer. PDLLA is usually amorphous and has a glass transition temperature of about 56°C. In vivo results of PDLLA screws demonstrated that these screws would not be degraded at least for 6 weeks, but they would be completely absorbed by the body in 10 months [50]. All PDLLA, PLLA, and PGA copolymers could provide different mechanical properties together and none of them has this capability by itself. For example, the glass transition temperature of PDLLA/PGA blend with 50:50

portions is about 30°C and increasing the PDLA: PGA ratio from 65:35 to 75:25 leads to an increase in the T_g temperature from 33.3°C to 38°C [51]. A blend of PDLA and PGA with the ratio of 82:18 (Lactosorb, Biomet sport medicine, Inc., Warsaw, In) can provide a nanocrystalline copolymer with a temperature of 55.3°C T_g . It was found that a 2°C increase in T_g temperature would significantly increase the hydrolysis degradation rate of lactosorb from 20% to 25% [52]. Moreover, blending PDLA with 10, 20, and 30% wt of PCL phase decreased T_g PDLA from 67.3°C to 66.2, 65.1, and 63.5 °C, respectively [53].



Figure 4. Creation of secure fit by holding of screw between the graft bone plug and the wall of the drilled hole [15]

PDLA/PCL blends reinforced with Bioactive Glass nanoparticles (BGn) showed that the addition of BGn improved the initial mechanical properties as well as biological activity [54].

Phusilin biodegradable interference screws (poly-D(2%), L(98%)-lactide, Phusis, Saint-Ismier, France) are used in patella tendon autograft fixation. The results of an average follow-up of 24 months showed that screws were degraded while bone in-grows earlier than an individual PLLA screw. Clinical tests and MRI results showed no adverse complications during screw insertion thanks to its degradation [52]. The tin octoate is commonly used as an initiator of PDLA polymerization; however, in order to decrease body immune response to implant screws in phusilin screws, polymerization process is applied to ring-opening procedure using zinc catalyst, which consists of less toxic material. Ring-opening polymerization that uses zinc as a polymerization initiator creates a combination of stereoisomers by means of ionic reactions. In this case, the resulting screws are more hydrophilic than the PLA screws derived from tin and can create interference screws with quicker degradation [52].

Bioabsorbable interference screws (Sysorb; Sulzer Orthopedics, Baar, Switzerland) are used for autologous

BPTB fixation through the press-fit technique and distal bone block in 25 patients. The results showed that no replacement of sysorb screws in tibial tunnel took place by osseous neo-formation up to 8 months after ACLR surgery, excluding one performed on tibial bone tunnel enlargement and tibial subcutaneous cyst [55]. Mechanical evaluations of Sysorb screws used for BPTB graft fixation in cadaver indicated that the maximum pull-out force and toughness were 544±109 N and 162±27 N/mm, respectively. Cyclical loading elongation also showed that during the first five cycles, 5th-20th, and 20th-1500th loading cycles, the amounts of elongations reached 1.4 mm, 0.14 mm, and 4.1mm, respectively [56].

Biological ACLR screws (85/15 PDLA/PGA, Instrument Maker, Inc., Okemos, MI) revealed some pieces of evidence of total screw degradation, bone remodeling, and new bone formation in femoral and tibial bone tunnel throughout a two-year follow-up. Moreover, MRI results showed no cystic or osteolytic changes associated with minimum swelling at the implant site [57]. Studies of biodegradable screws megfix (70/30 PLLA-PDLA, Storz-Endoscope Tuttlingen, Germany) with three different diameters of 6, 7, and 8 mm implanted in porcine knee showed that none of 6mm screws, 3 of 7 mm screws, and all the 8 mm screws were able to tolerate cyclical loading protocol. Elongations after 1000 cyclic load achieved 8.36 and 4.26 mm for 7 mm and 8 mm screws, respectively. The maximum load, yield strength, and toughness for 7 mm screws were 245 N, 199.1 N, and 98.6 N/mm, respectively. These values for 8 mm screws were 567 N, 456.9 N, and 151 N/mm, respectively [58].

4.3. POLYMER/TRI-METHYL CARBONATE (TMC) ACL SCREWS

TMCs with elastic properties similar to rubbery polymers are not appropriate for biomedical application, because they are characterized by poor dimensional stability, tackiness, and inadequate mechanical properties [59]. However, the combination of TMC and other polymers like PGA, PLLA, and PDLA could create interesting biomechanical properties that will be favorable for particular applications. As an example, Polyglyconate is a block copolymer of glycolic acid and TMC linked together by covalent bonding. Copolymers of PGA and TMC have more flexibility than PGA alone. In vitro studies have shown that the molecular weight of unirradiated PGA cultured in PBS solution decreased from 124 kDa to 18.6 kDa for 31 days. The ultimate tensile strength of unirradiated PGA falls down from 51.7 MPa to 5.7 MPa after 3 weeks [60]. However, results of in vivo studies of polyglyconate implants revealed that their mechanical properties and integrity disappeared within 6 weeks and the full resorption of implant took place within 6 to 12 months [61]. Comparative in vivo studies were performed on 20

patients who had femoral bone block fixation with a bioabsorbable interference screw (EndoFix absorbable interference screw; Smith & Nephew Endoscopy, Andover, MA) and tibial bone block fixation with a titanium screw. The follow-up results of 3, 6, 12, and 24 months indicated no problem and complications related to graft fixation took place for bioabsorbable as well as titanium screws. Upon the point of 12 months, degradation of the implant was complete, whereas there was no radiological evidence of bony replacement up to 3 years postoperation [30]. ACL hexagon Inion screws (PDLLA- TMC, Inion Ltd., Tampere, Finland) illustrated that they preserved 70% to 90% of their initial strength during 12 weeks and considerable degradation during 18 to 36 weeks, whereas complete degradation took place up to 2 years, post operation [62]. MRI results of 2 follow-up years indicated that the screw degraded bone tunnels replaced by fibrosis like tissues. Initial fixation strength of Hexalon Inion screws was evaluated at three separate levels in comparison to (i) interference metallic screws for fixation of soft tissue graft, (ii) smart self-reinforced screws for fixation of soft tissue grafts, and (iii) PLLA bioscrews used for fixation of bone-tendon-bone grafts. Yield loads of Hexalon Inion screws in each experiment were obtained as 491 N, 501 N, and 901 N, respectively [63,64]. Hence, researchers found that the strength of Hexalon Inion screws was similar to that of other polymeric and metallic screws .

5. BIOACTIVE AND BIOABSORBABLE COMPOSITE ACL SCREWS

5.1. EFFECTS OF BONE MINERAL PHASES IN ACLR SCREWS

Incorporation of various inorganic phases such as calcium carbonate (CC), β -tricalcium phosphate (β -TCP), and hydroxyapatite (HA) into ACLR screws compositions could overcome some shortcomings of other polymeric ACLR screws. Addition of these phases to ACLR screw compositions could enhance the absorption rates of bioabsorbable screws, treat osteogenesis after absorption, reduce oxidation, and act as buffering agents to reduce the acidity of screw adjacent resulting from the decomposition products of screws based on polymers with the acidic origin.

A comparative clinical and radiological study was conducted on 349 patients between 2 different tibial fixations performed using bioabsorbable poly-L-lactide (PLLA) and PLLA-HA ACL screws. The results showed that the PLLA-HA screw groups would induce a significant reduction in the tibial tunnel widening and foreign body reactions, improving the osteointegration and significantly increasing screw resorption compared to the pure PLLA group [65]. The proximal tibial tunnel widening effects of PLLA groups revealed a positive

correlation with knee laxity. Hunt and Callaghan carried out an in vitro animal study to compare a composite (PLLA-HA) with PLLA screw. They concluded that the composite screw significantly increased new bone formation and decreased inflammatory reactions in comparison with the PLLA screw [66]. The Computed Tomography (CT) evaluations demonstrated that the pure PLLA screws were completely degraded after 5 years with no evidence of osteoconductivity behavior, leaving bone void after degradation [67]. In the meantime, biocomposites screws made of PLLA (70%)/ β -TCP (25%) (Bilok, ArthroCare, Sunnyvale, CA) and copolymer of 70 % PLLA/PGA with 30% β -TCP (Milagro, DePuy Mitek) showed complete degradation and osteoconductivity at 75% and 81% of the screw sites and complete filling of screw void in 10% and 19% of tests, respectively [68].

It was found that the content of mineral bone phase could also affect the degradation rate of screws and osteoconductivity behaviors. Research on two different amounts (30% and 60%) of β -TCP evaluated using CT scans over 29 to 45 months showed that the biocomposite of PLLA/30 % β -TCP (Ligafix; SBM, Lourdes, France) exhibited more dominant osteoconductivity behavior than other screws containing 60 % β -TCP [69]. This is due to at least two reasons: (a) the screws with greater β -TCP content were absorbed more rapidly; (b) the screws with 30 % β -TCP could be completely surrounded by bone plug or tibial bone rather than screws containing 60% β -TCP [70]. The other theory in this respect depicts the greater release of phosphate ions into the adjacent screw during degradation by screws with high β -TCP, resulting in a greater pH which may play an inhibitory role in the osteoconductivity manners [70].

5.2. POLYLACTIDE CARBONATE ACL SCREWS

Calcium Carbonate (CC) is a bone mineral phase that forms other bone calcium salts. A combination of CC and other polymeric materials would create an osteoconductive interface that may provide enhanced degradation properties and stimulate its replacement by new bone formation [71]. The presence of calcium carbonate into implants could also provide pH value between 7.4 and 6.3 throughout the degradation process; help avoid local acidity formation [72]. An interference screw made from a novel bioabsorbable material, polylactide carbonate (PLC) (Calaxo Screw; Smith & Nephew Endoscopy, Andover, MA) is composed of PGA and PDLLA (65%) copolymers at ratio of 85:15 and 35% calcium carbonate. The combination of PDLLA-co-PGA and calcium carbonate is an appropriate composite material for ACLR screws. In vitro studies and molecular weight (M_w) changes surveying of calaxo screws into phosphate buffer saline (PBS, pH=7.36) for following up to 12 weeks was performed. The results suggested that the calaxo screws

lost 85% of its molecular weight, whereas pH of PBS also decreased to 6.86 [73]. Researchers found that the buffering effect of CC may lead to rapid degradation of screws. The *in vivo* studies of calaxo screws carried out by insertion of ACLR screws into 41 sheep. No inflammatory reaction was realized with a mean follow-up of 6, 12, 26, and 52 weeks after implantation into sheep body. Within 26 weeks after insertion, screws partially were replaced by new bone; however, in 52 weeks after implantation, they were resorbed completely, whereas they were simultaneously replaced with a new bone. The ultimate load to failure of these screws was identified 70 N and 225 N for 6 and 12 weeks after implantation, respectively [71].

5.3. POLYMERIC COMPOSITES ACL SCREWS WITH β -TRICALCIUM PHOSPHATE

Various companies designed the ACL screws made of polymer-based composites reinforced by osteoconductive and osteoinductive phases. For example, biodegradable screws contain PDLLA, PLLA, and PLGA as polymeric and β -tricalcium phosphate (β -TCP) as osteoinductive materials. β -TCP has brittle origin with low toughness, this means that the susceptibility of cracks formation throughout the brittle materials restrict the capability of these materials for load-bearing applications. These materials presented good osteoconductive properties and hydrolytic dissolution products of materials that contain calcium and phosphate ions [74]. Adding β -TCP to PLLA screws improved the mechanical properties and also observed that β -TCP caused an increase in both the degradation kinetics of the composite material, accelerating the remodeling and healing of bone. Moreover, β -TCP is alkaline in solution and may neutralize the acidic by-product resulting from PLLA degradation. A PLGA screw has more rapid degradation than PLLA one that can, in combination with β -TCP, provide a proper degradation profile as well as osteoconductive and osteoinductive properties due to the presence of TCP phase. There are some ACL screws composed of TCP phase. For example, Bio-intrafix screws made of 30% β -TCP and 70% PLLA [75]. *In vivo* studies of Bio-intrafix screws administered to the body of patients illustrated that no post-surgery adverse inflammatory reaction occurred up to 2 years. In addition, the ultimate tensile strength of Bio-intrafix screws indicated about 700 N [76]. In this respect, another screw is composed of 30% β -TCP and 70% PLGA (Biocryl, Rapide TM). Preclinical *in vivo* studies illustrated that the composite-based screws inserted into cortical femoral bone defect were completely degraded throughout 24 months and simultaneously replaced with a new bone [77]. Another *in vitro* studies on Biocryl screws were carried out in PBS solution with pH=7.36. The results showed that the dimensional variations of the screw occurred to some extent after 12 weeks from

culturing into PBS solution [73]. Throughout this time, molecular weight decreased to 66.9%, whereas pH almost unchanged. These results proved that TCP might increase the degradation rate of Biocryl screws. This may be due to the alkaline origin of TCP materials, which could make a buffering circumstance for acidic by-products resulting from screw degradation. These screws in another study were used as ACL screws in tibial bone tunnel enlargement. Tibial fixation was performed using 2 bioresorbable interference screws. Magnetic Resonance Imaging (MRI) was performed on all patients after 1 year post operation. The results determined an increase in bone tunnel enlargement up to 43% by digitally measuring the widths of the bone tunnel perpendicular to the long axis of the tunnels on an oblique coronal and axial planes. However, there is no report about the degradation profile of screws [78]. Another study investigated the biodegradable β -TCP-PLGA screws for fixation of ACL autograft patellar tendon inserted into 41 patients. During the follow-up 3 years, the post operative results illustrated that complete degradation accompanied by new bone formation occurred. The degradation rate of β -TCP-PLGA based screws was more than that of the β -TCP-PLLA screw [73].

5.4. POLYMERIC COMPOSITE SCREWS WITH HYDROXYAPATITE



Hydroxyapatite (HA) similar to β -TCP is a bioceramic inorganic material and a major constituent of bone whose high biocompatibility has been widely used for bone remodeling [79]. Besides, HA can act as a buffering factor against acidic products resulting from PLLA degradation. Similar to β -TCP, HA suffers from low fracture toughness and also high brittleness. Elastic modulus of HA varied from 80 to 100 GPa and its compressive strength ranged from 500 to 1000 MPa [75]. *In vitro* studies of PLLA/HA composite material in PBS solution with pH= 7.36 were introduced such that no significant changes occurred throughout the 12 weeks; however, the molecular weight of screws decreased by about 22.9% and pH also slightly decreased from 7.36 to 7.32 [73]. Two biodegradable ACL screws, i.e., PLLA-HA composite screws and no composite PLLA screws, were compared. The results of evaluation studies showed that the remaining strength of HA-PLLA composite after 24 weeks is higher than PLLA screws. Modulus of composite screw was also more similar to that of natural bone tissue. This similarity between composite screws and natural bone tissue modulus causes a substantial decrease in stress shielding during the bone healing [80]. A study was performed on BIORCI-HA screws made of HA-PLLA composite for fixation of patellar tendon graft into 20 patients. Based on MRI images of screws inserted into the body, no complication during the 2-year follow-up and inflammatory reaction at patellar tendon graft were

observed. Although the degradation rate of screws and bone integration were slow based on MRI, it should be noted that in this study, screw failure during insertion was just reported in one patient [81].

6. MAGNESIUM AND MAGNESIUM ALLOYS AS POTENTIAL BIODEGRADABLE ACL SCREWS

Non-degradable titanium interference screws may impair the tendon or ligament graft throughout the screw insertion. This may be due to high mechanical strength. Besides, these screws need a second surgery for removal. In the case of bioabsorbable ACLR screws as a well-established practice, there also are some complications. As an example, due to inadequate mechanical strength, the screw may fail upon insertion. In addition, during the degradation process, some adverse reactions such as synovitis, granuloma, and tunnel enlargement may occur, retarding the healing of tendon grafts by fibrous scar tissue layer formation at the tendon-bone interface [82,83]. In this respect, biodegradable metallic screws with modulus resembling the natural bone can be a proper choice. Recently, magnesium (Mg) and Mg alloys represented an interesting potential for biomedical application and may be suitable for tendon graft fixation in ACLR reconstruction as a new generation of bioactive implants [38,84-85]. These screws could stimulate fibrocartilage regeneration. Additionally, these types of screws possess a good mechanical behavior owing to their similarity in modulus between Mg (41-45 GPa) and natural bone (15-25 GPa) [86], which could meet strength requirements throughout the insertion into bone. Mg metal could be degraded when exposed to the aqueous solution. Its degradation is initiated by chemical reaction with body fluid and release of the Mg ions and equivalent mole of hydrogen gas.

Generally, Mg is firstly oxidized throughout the anodic reactions to formations and then, throughout a cathodic reaction, the water of body fluid is reduced by the generated electrons during the last levels. Furthermore, $Mg(OH)_2$ is formed as the overall products. Dissolution of passive $Mg(OH)_2$ layers in the presence of destructive biological ions such as Cl^- ions occurs according to Equation 4. Furthermore, the degradation of Mg implants into body environments including Cl^- ions is dominant because the degradation rate of the passive layer is higher than that of degrading products on the surface [87].



Since the Mg ions have a stimulating role in osteogenic differentiation of stem cells, it could promote the osseous ingrowth into graft as well as the incorporation of tendon graft into the surrounding bone tissue enhancement [88]. Most recently, Cheng et al. introduced the high purity Mg as promising materials for use of interference ACL screws [23]. They also expressed that Mg interference screws could effectively inhibit the degeneration of the tendon graft by reducing the expression level of MMP-13, while the remodeling phase occurred. This fact indicates that more collagen fibers in the tendon graft were preserved to connect the surrounding bone tissue for higher knee stability [89]. However, it has not been yet reported if Mg-based implants could also promote graft healing in tendon-bone healing in a bone tunnel [25]. Besides, there is no sufficient information about the bone tunnel after surgery to determine the potential application of Mg implants. Therefore, it seems that the investigation of graft healing quality into bone tunnel in ACLR reconstruction model is crucial. Herein, it was hypothesized that Mg-based interference screw could significantly enhance the incorporation of tendon graft within a bone tunnel when compared to conventional Ti interference screws.

7. MECHANICAL PROPERTIES OF ACLR SCREWS

The ACLR screws intend to fix ligament into tibial or femoral bones that must have sufficient mechanical strength when either inserted into the bone tunnel during surgery or fixed the ligament into the bone for a certain time until rehabilitation of damaged ligament is completed. Regarding the initial fixation strength of ACLR screws, many factors such as bone quality and its diameter and screw features such as length, diameter, design, and material compositions are affected. Moreover, the age of patients and surgery techniques affect the mechanical properties of implanted ACLR screws. In terms of screw geometry, there are many controversies with respect to the appropriate diameter and length of screws on mechanical strength. It was found that an increase in screw diameter could increase the fixation strength [90]. There is also hypothesized over the screw length effects on biomechanical properties. In one study, it was found that the significant improvement of the mechanical properties of BPTB units was made when they were fixed with a custom-designed 9 mm interference screw rather than a 6.5 mm cancellous screw [47]. Moreover, use of fully-threaded ACL screws has remarkably increased the fixation strength rather than partially-threaded screws [47].

In terms of material compositions, several attempts have been made to develop biodegradable ACLR screws with sufficient strength for the fixation of ligament or tendon

into bone tunnel. The weakness of graft fixation immediately and during the first six to eight weeks after surgery will limit early intensive rehabilitation [91]. In a study where the fixation strength of PLLA biodegradable screws compared with two metal screws, the results show that there is no significant difference among the three groups. Therefore, the mean forces to failures in the three groups of metal interference (n=11), an AO cancellous screw (n=11), and PLLA screws (n=11) were 1358 ± 348 N, 1081 ± 331 N, and 1211 ± 362 N, respectively [47].

Regarding screw insertion during operation, since the screw was submitted to torsional and axial loads owing to the application of compression and longitudinal shear forces [92], it has been reported that the biodegradable screws may be subjected to break during operation [93]. The technical standard ASTM F2502 (Standard Specification and Test Methods for Bioabsorbable Plates and Screws for Internal Fixation Implants) provides a standard test method for measuring the mechanical properties of polymer screws in torsion [94]. According to this standard, the fully threaded screw was equipped with the holding device so that five threads under the head of the screw were exposed outside the holding device. A large enough portion of the screw thread should be gripped firmly to secure the screw so that it does not rotate when exposed to torsion loads. The torque is applied by inserting the screw driver (bit) into the screw head. However, unlike solid core osteosynthesis screws, cannulated interference bioabsorbable screws have a cylindrical orifice along almost their entire length to the screw driver connection [95].

Torsion test results of PLDLA 70/30 screws during hydrolysis circumstance identify that the mechanical behavior of screws switched from ductile to fragile as a function of degradation time up to 240 days. The results demonstrated that the maximum torque varied from 1168 N.mm to 349 N.mm after 240 days, whereas the maximum torque angle varied from 85.42 to 8.28 degrees. Moreover, the torsional stiffness of screws decreased from 70 Nmm/deg to 54 Nmm/deg [94].

A novel hydroxyapatite ACL screw with a novel geometry presented by Schumacher et al. showed that the application of multiple threads with a large thread pitch to screw design facilitated the insertion of the screws into the bone without the application of screw driver or an external torque. Besides, the *ex vivo* studies of screws with rigid polyurethane (PU) foam and sheep ankle showed the pull-out forces of 486 ± 60 N and 387 ± 160 N, respectively, and these values are comparable to commercially BioComposite interference screws (Arthrex Inc., Germany) tested in PU foam, i.e., 435 ± 120 N [96].

Another research group performed a comparison between bioabsorbable screws (self-reinforced L-lactide/D-lactide, PLA 96/4, Bionx Implant Ltd., Tampere Finland) and titanium interference (Softsilk, Acufex Microsurgical Inc., Mansfield, Massachusetts) ones in ACL reconstruction using matched pairs of porcine knees. For this reason, two groups of screws were used in single and cyclic loading conditions [97]. The results showed that the mean ultimate failure loads for the single-cycle failure loading test were 837 ± 260 N and 863 ± 192 N for the bioabsorbable and titanium interference screws, respectively (no significant difference). Moreover, the yield loads were obtained as 605 ± 142 N and 585 ± 103 N for the bioabsorbable and titanium interference screws, respectively (no significant difference) [97].

For the sake of comparison, the characteristics of biomechanical properties for the ACL screws studied in the current review paper and other commercial screws are summarized in Table 2.

8. CONCLUSION

There are two different categories of ACL screws, namely metallic and bioabsorbable. The mechanical, physical, chemical composition, insertion technique, and various manufacturers as well as *in vivo* behaviors of different biodegradable commercial ACL screws were investigated in this research. The findings illustrated that the bioabsorbable screws showed similar behaviors to the metallic ones in several cases. However, the bioabsorbable screws suffer from some drawbacks, especially in bone ingrowth that prevents them from leaving a void after disappearing. Generally, the commercial bioabsorbable ACL screws are currently composed of polymers such as PLA and the enantiomers, PGA, PCL, and in some cases, composites of these polymers with inorganic filler phases such as Ca-P based products. Incorporation of bone mineral phases into ACLR screws may enhance the absorption rates of bioabsorbable screws, lessen the chances of osteogenesis, help neutralize the environs of bone site, and improve the mechanical properties.

The potential new generation of these screws may be magnesium screws and they have not reached their commercial production objective.

Given the literature reviews, the authors hold the belief that the biocomposite ACL screws rather than polymeric and metallic ones possess interesting features in terms of biological, physical, and mechanical properties. However, there are some challenges such as the optimum contents of bioceramics on osteogenesis and mechanical properties.

TABLE 2. Comparison of mechanical properties of commercial ACLR screws

Screws Compositions	Manufacturer	Screws Dimensions	Ultimate Failure Load	Yield Point Load	Ref.
			(N)	(N)	
30% β -TCP/70% PLLGA	DePuy	10 \times 35 mm	1113 \pm 362.2	845.1 \pm 243.7	[95]
30% BCP/70% PDLA	Arthrex	10 \times 35 mm	1051 \pm 244.5	792.2 \pm 157.5	[95]
70% PLGA/30% β -TCP	Milagro(DePuy)	10 mm	877 \pm 8	728	[98]
25% HA/75% PLLA	Smith & Nephew	10 \times 35 mm	920.3 \pm 283.5	684.1 \pm 163.9	[95]
70% PLDLA/30% BCP	BioComposite (Arthrex)	10 mm	1206 \pm 248	1053 \pm 378	[98]
Self-Reinforced L-lactide/D-lactide (PLA 96/4)	Bionx Implant Ltd., Tampere, Finland	7 \times 25 mm	837 \pm 260	621 \pm 139	[99]
25% HA/75% PLLA	Srtyker	10 \times 35 mm	1073.8 \pm 378.7	797.6 \pm 293.3	[95]
PLLA/TCP	Suspension screw (Bilok ST screw, Biocomposites Ltd, Etruria, UK)	9 \times 35 mm	1475	998.5	[49]
PLLA/TCP	Interference Screw (Bilok TS; Biocomposites Ltd)	9 \times 30 mm	652	538	[49]
PLLA	Arthrex, Naples, FL	7 \times 23 mm	995	689	[43]
PLLA 70/30	Linvatec, Largo, Florida- USA	9 \times 20 mm	607.11 \pm 97.49	509.98 \pm 94.03	[100]

REFERENCES

1. Fineberg, M. S., Zarins, B., Sherman, O. H., "Practical considerations in anterior cruciate ligament replacement surgery", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 16, No. 7, (2000), 715-724. <https://doi.org/10.1053/jars.2000.8951>
2. Lee, J. W., Han, H. S., Han, K. J., Park, J., Jeon, H., Ok, M. R., Seok, H. K., Ahn, J. P., Lee, K. E., Lee, D. H., Yang, S. J., "Long-term clinical study and multiscale analysis of in vivo biodegradation mechanism of Mg alloy", *Proceedings of the National Academy of Sciences*, Vol. 113, No. 3, (2016), 716-721. <https://doi.org/10.1073/pnas.1518238113>
3. Zhao, D., Huang, S., Lu, F., Wang, B., Yang, L., Qin, L., Yang, K., Li, Y., Li, W., Wang, W., Tian, S., "Vascularized bone grafting fixed by biodegradable magnesium screw for treating osteonecrosis of the femoral head", *Biomaterials*, Vol. 81, (2016), 84-92. <https://doi.org/10.1016/j.biomaterials.2015.11.038>
4. Staiger, M. P., Pietak, A. M., Huadmai, J., Dias, G., "Magnesium and its alloys as orthopedic biomaterials: a review", *Biomaterials*, Vol. 27, No. 9, (2006), 1728-1734. <https://doi.org/10.1016/j.biomaterials.2005.10.003>
5. Sumner, D. R., Galante, J. O., "Determinants of stress shielding: design versus materials versus interface", *Clinical Orthopaedics and Related Research*, Vol. 274, (1992), 202-212. <https://doi.org/10.1097/00003086-199201000-00020>
6. Cutright, D. E., Hunsuck, E. E., "Tissue reaction to the biodegradable polylactic acid suture", *Oral Surgery, Oral Medicine, Oral Pathology*, Vol. 31, No. 1, (1971), 134-139. [https://doi.org/10.1016/0030-4220\(71\)90044-2](https://doi.org/10.1016/0030-4220(71)90044-2)
7. Konan, S., Haddad, F. S., "A clinical review of bioabsorbable interference screws and their adverse effects in anterior cruciate ligament reconstruction surgery", *The Knee*, Vol. 16, No. 1, (2009), 6-13. <https://doi.org/10.1016/j.knee.2008.06.001>
8. Lambert, K. L., "Vascularized patellar tendon graft with rigid internal fixation for anterior cruciate ligament insufficiency", *Clinical Orthopaedics and Related Research (1976-2007)*, Vol. 172, (1983), 85-89. <https://doi.org/10.1097/00003086-198301000-00016>
9. Kurosaka, M., Yoshiya, S., Andrich, J. T., "A biomechanical comparison of different surgical techniques of graft fixation in anterior cruciate ligament reconstruction", *The American Journal of Sports Medicine*, Vol. 15, No. 3, (1987), 225-229. <https://doi.org/10.1177/036354658701500306>
10. Almazán, A., Miguel, A., Odor, A., Ibarra, J. C., "Intraoperative incidents and complications in primary arthroscopic anterior cruciate ligament reconstruction", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 22, No. 11, (2006), 1211-1217. <https://doi.org/10.1016/j.arthro.2006.06.019>
11. Matthews, L. S., Soffer, S. R., "Pitfalls in the use of interference screws for anterior cruciate ligament reconstruction: brief report", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 5, No. 3, (1989), 225-226. [https://doi.org/10.1016/0749-8063\(89\)90177-1](https://doi.org/10.1016/0749-8063(89)90177-1)
12. Böstman, O. M., Pihlajamäki, H. K., "Adverse tissue reactions to bioabsorbable fixation devices", *Clinical Orthopaedics and Related Research (1976-2007)*, Vol. 371, (2000), 216-227. <https://doi.org/10.1097/00003086-200002000-00026>
13. Bottoni, C. R., DeBerardino, T. M., Fester, E. W., Mitchell, D., Penrod, B. J., "An intra-articular bioabsorbable interference screw mimicking an acute meniscal tear 8 months after an anterior cruciate ligament reconstruction", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 16, No. 4, (2000), 395-398. [https://doi.org/10.1016/S0749-8063\(00\)90085-9](https://doi.org/10.1016/S0749-8063(00)90085-9)
14. Barber, F. A., Boothby, M. H., "Bilok interference screws for anterior cruciate ligament reconstruction: clinical and radiographic outcomes", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 23, No. 5, (2007), 476-481. <https://doi.org/10.1016/j.arthro.2006.12.026>

15. Davis, K., Huser, A., Kreofsky, C., Nadler, D., Poblocki, J., "Bioactive Interference Screw for ACL Reconstruction", *Biomedical Engineering Design* 400, University of Wisconsin-Madison. December 7, (2005). <http://130.203.136.95/viewdoc/download?doi=10.1.1.456.6058&rep=rep1&type=pdf>
16. Watson, J. N., McQueen, P., Kim, W., Hutchinson, M. R., "Bioabsorbable interference screw failure in anterior cruciate ligament reconstruction: a case series and review of the literature", *The Knee*, Vol. 22, No. 3, (2015), 256-261. <https://doi.org/10.1016/j.knee.2015.02.015>
17. Moisala, A. S., Järvelä, T., Paakkala, A., Paakkala, T., Kannus, P., Järvinen, M., "Comparison of the bioabsorbable and metal screw fixation after ACL reconstruction with a hamstring autograft in MRI and clinical outcome: a prospective randomized study", *Knee Surgery, Sports Traumatology, Arthroscopy*, Vol. 16, No. 12, (2008), 1080-1086. <https://doi.org/10.1007/s00167-008-0593-z>
18. Mayr, H. O., Hube, R., Bernstein, A., Seibt, A. B., Hein, W., von Eisenhart-Rothe, R., "Beta-tricalcium phosphate plugs for press-fit fixation in ACL reconstruction—a mechanical analysis in bovine bone", *The Knee*, Vol. 14, No. 3, (2007), 239-244. <https://doi.org/10.1016/j.knee.2007.01.006>
19. Arama, Y., Salmon, L. J., Sri-Ram, K., Linklater, J., Roe, J. P., Pinczewski, L. A., "Bioabsorbable versus titanium screws in anterior cruciate ligament reconstruction using hamstring autograft: a prospective, blinded, randomized controlled trial with 5-year follow-up", *The American Journal of Sports Medicine*, Vol. 43, No. 8, (2015), 1893-1901. <https://doi.org/10.1177/0363546515588926>
20. Gulick, D. T., Yoder, H. N., "Anterior cruciate ligament reconstruction: clinical outcomes of patella tendon and hamstring tendon grafts", *Journal of Sports Science & Medicine*, Vol. 1, No. 3, (2002), 63-71.
21. Laxdal, G., Kartus, J., Eriksson, B. I., Faxen, E., Sernert, N., Karlsson, J., "Biodegradable and metallic interference screws in anterior cruciate ligament reconstruction surgery using hamstring tendon grafts: prospective randomized study of radiographic results and clinical outcome", *The American Journal of Sports Medicine*, Vol. 34, No. 10, (2006), 1574-1580. <https://doi.org/10.1177/0363546506288014>
22. Shen, C., Jiang, S. D., Jiang, L. S., Dai, L. Y., "Bioabsorbable versus metallic interference screw fixation in anterior cruciate ligament reconstruction: a meta-analysis of randomized controlled trials", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 26, No. 5, (2010), 705-713. <https://doi.org/10.1016/j.arthro.2009.12.011>
23. Cheng, P., Han, P., Zhao, C., Zhang, S., Wu, H., Ni, J., Hou, P., Zhang, Y., Liu, J., Xu, H., Liu, S., "High-purity magnesium interference screws promote fibrocartilaginous entheses regeneration in the anterior cruciate ligament reconstruction rabbit model via accumulation of BMP-2 and VEGF", *Biomaterials*, Vol. 81, (2016), 14-26. <https://doi.org/10.1016/j.biomaterials.2015.12.005>
24. Bach, F. D., Carlier, R. Y., Elis, J. B., Mompont, D. M., Feydy, A., Judet, O., Beaufils, P., Vallée, C., "Anterior cruciate ligament reconstruction with bioabsorbable polyglycolic acid interference screws: MR imaging follow-up", *Radiology*, Vol. 225, No. 2, (2002), 541-550. <https://doi.org/10.1148/radiol.2252010357>
25. Bedi, A., Kawamura, S., Ying, L., Rodeo, S. A., "Differences in tendon graft healing between the intra-articular and extra-articular ends of a bone tunnel", *HSS Journal*, Vol. 5, No. 1, (2009), 51-57. <https://doi.org/10.1007/s11420-008-9096-1>
26. Morgan, C. D., Gehrman, R. M., Jayo, M. J., Johnson, C. S., "Histologic findings with a bioabsorbable anterior cruciate ligament interference screw explant after 2.5 years in vivo", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 18, No. 9, (2002), 1-6. <https://doi.org/10.1053/jars.2002.36466>
27. Park, M. C., Tibone, J. E., "False magnetic resonance imaging persistence of a biodegradable anterior cruciate ligament interference screw with chronic inflammation after 4 years in vivo", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 22, No. 8, (2006), 911-e1. <https://doi.org/10.1016/j.arthro.2005.06.030>
28. Warden, W. H., Chooljian, D., Jackson, D. W., "Ten-year magnetic resonance imaging follow-up of bioabsorbable poly-L-lactic acid interference screws after anterior cruciate ligament reconstruction", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 24, No. 3, (2008), 370-e1. <https://doi.org/10.1016/j.arthro.2006.12.032>
29. Barber, F. A., Elrod, B. F., McGuire, D. A., Paulos, L. E., "Bioscrew fixation of patellar tendon autografts", *Biomaterials*, Vol. 21, No. 24, (2000), 2623-2629. [https://doi.org/10.1016/s0142-9612\(00\)00130-7](https://doi.org/10.1016/s0142-9612(00)00130-7)
30. Fink, C., Benedetto, K. P., Hackl, W., Hoser, C., Freund, M. C., Rieger, M., "Bioabsorbable polyglyconate interference screw fixation in anterior cruciate ligament reconstruction: a prospective computed tomography-controlled study", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 16, No. 5, (2000), 491-498. <https://doi.org/10.1053/jars.2000.4633>
31. Hackl, W., Fink, C., Benedetto, K. P., Hoser, C., "Transplant fixation by anterior cruciate ligament reconstruction. Metal vs. bioabsorbable polyglyconate interference screw. A prospective randomized study of 40 patients", *Der Unfallchirurg*, Vol. 103, No. 6, (2000), 468-474. <https://doi.org/10.1007/s001130050567>
32. Kaeding, C., Farr, J., Kavanaugh, T., Pedroza, A., "A prospective randomized comparison of bioabsorbable and titanium anterior cruciate ligament interference screws", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 21, No. 2, (2005), 147-151. <https://doi.org/10.1016/j.arthro.2004.09.012>
33. Marti, C., Imhoff, A. B., Bahrs, C., Romero, J., "Metallic versus bioabsorbable interference screw for fixation of bone-patellar tendon-bone autograft in arthroscopic anterior cruciate ligament reconstruction A preliminary report", *Knee Surgery, Sports Traumatology, Arthroscopy*, Vol. 5, No. 4, (1997), 217-221. <https://doi.org/10.1007/s001670050053>
34. Myers, P., Logan, M., Stokes, A., Boyd, K., Watts, M., "Bioabsorbable versus titanium interference screws with hamstring autograft in anterior cruciate ligament reconstruction: a prospective randomized trial with 2-year follow-up", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 24, No. 7, (2008), 817-823. <https://doi.org/10.1016/j.arthro.2008.02.011>
35. Shen, P. H., Lien, S. B., Shen, H. C., Wang, C. C., Huang, G. S., Chao, K. H., Lee, C. H., Lin, L. C., "Comparison of different sizes of bioabsorbable interference screws for anterior cruciate ligament reconstruction using bioabsorbable bead augmentation in a porcine model", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 25, No. 10, (2009), 1101-1107. <https://doi.org/10.1016/j.arthro.2009.05.011>
36. Drogset, J. O., Grøntvedt, T., Tegnander, A., "Endoscopic reconstruction of the anterior cruciate ligament using bone-patellar tendon-bone grafts fixed with bioabsorbable or metal interference screws: a prospective randomized study of the clinical outcome", *The American Journal of Sports Medicine*, Vol. 33, No. 8, (2005), 1160-1165. <https://doi.org/10.1177/0363546504272264>
37. Papalia, R., Vasta, S., D'Adamio, S., Giacalone, A., Maffulli, N., Denaro, V., "Metallic or bioabsorbable interference screw for graft fixation in anterior cruciate ligament (ACL) reconstruction?", *British Medical Bulletin*, Vol. 109, No. 1, (2014), 19-29. <http://doi.org/10.1093/bmb/ldt038>

38. Wang, J., Xu, J., Song, B., Chow, D. H., Yung, P. S. H., Qin, L., "Magnesium (Mg) based interference screws developed for promoting tendon graft incorporation in bone tunnel in rabbits", *Acta Biomaterialia* Vol. 63, (2017), 393-410. <http://doi.org/10.1016/j.actbio.2017.09.018>
39. Chen, C. H., Lee, C. H., "Biological fixation in anterior cruciate ligament surgery", *Asia-Pacific Journal of Sports Medicine, Arthroscopy, Rehabilitation and Technology*, Vol. 1, No. 2, (2014), 48-53. <http://doi.org/10.1016/j.asmart.2014.02.004>
40. Kohn, J., Abramson, S., Langer, R., "Bioresorbable and bioerodible materials", In Ratner, B. D., Hoffman, A. S., Schoen, F. J., Lemons, J. E. (eds), *Biomaterials Science: An Introduction to Materials in Medicine*, Elsevier Academic Press, San Diego, (2004), 115-127.
41. Urayama, H., Kanamori, T., Kimura, Y., "Microstructure and thermomechanical properties of glassy polylactides with different optical purity of the lactate units", *Macromolecular Materials and Engineering*, Vol. 286, No. 11, (2001), 705-713. [https://doi.org/10.1002/1439-2054\(20011101\)286:11<705::AID-MAME705>3.0.CO;2-Q](https://doi.org/10.1002/1439-2054(20011101)286:11<705::AID-MAME705>3.0.CO;2-Q)
42. Törmälä, P., "Biodegradable self-reinforced composite materials; manufacturing structure and mechanical properties", *Clinical Materials*, Vol. 10, No. 1-2, (1992), 29-34. [https://doi.org/10.1016/0267-6605\(92\)90081-4](https://doi.org/10.1016/0267-6605(92)90081-4)
43. Rupp, S., Krauss, P. W., Fritsch, E. W., "Fixation strength of a biodegradable interference screw and a press-fit technique in anterior cruciate ligament reconstruction with a BPTB graft", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 13, No. 1, (1997), 61-65. [https://doi.org/10.1016/s0749-8063\(97\)90210-3](https://doi.org/10.1016/s0749-8063(97)90210-3)
44. Caborn, D. N., Brand Jr, J. C., Nyland, J., Kocabey, Y., "A biomechanical comparison of initial soft tissue tibial fixation devices: the Intrafix versus a tapered 35-mm bioabsorbable interference screw", *The American Journal of Sports Medicine*, Vol. 32, No. 4, (2004), 956-961. <https://doi.org/10.1177/0363546503261696>
45. Chang, H. C., Nyland, J., Nawab, A., Burden, R., Caborn, D. N., "Biomechanical comparison of the bioabsorbable RetroScrew system, BioScrew XtraLok with stress equalization tensioner, and 35-mm Delta Screws for tibialis anterior graft-tibial tunnel fixation in porcine tibiae", *The American Journal of Sports Medicine*, Vol. 33, No. 7, (2005), 1057-1064. <https://doi.org/10.1177/0363546504272265>
46. Pena, F., Grøntvedt, T., Brown, G. A., Aune, A. K., Engebretsen, L., "Comparison of failure strength between metallic and absorbable interference screws: influence of insertion torque, tunnel-bone block gap, bone mineral density, and interference", *The American Journal of Sports Medicine*, Vol. 24, No. 3, (1996), 329-334. <https://doi.org/10.1177/036354659602400314>
47. Kousa, P., Jarvinen, T. L., Pohjonen, T., Kannus, P., Kotikoski, M., Jarvinen, M., "Fixation strength of a biodegradable screw in anterior cruciate ligament reconstruction", *The Journal of Bone and Joint Surgery. British Volume*, Vol. 77, No. 6, (1995), 901-905. <https://doi.org/10.1302/0301-620x.77b6.7593103>
48. Oh, Y. H., Namkoong, S., Strauss, E. J., Ishak, C., Jazrawi, L. M., Rosen, J., "Hybrid femoral fixation of soft-tissue grafts in anterior cruciate ligament reconstruction using the EndoButton CL and bioabsorbable interference screws: a biomechanical study", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 22, No. 11, (2006), 1218-1224. <https://doi.org/10.1016/j.arthro.2006.07.022>
49. Weimann, A., Rodieck, M., Zantop, T., Hassenpflug, J., Petersen, W., "Primary stability of hamstring graft fixation with biodegradable suspension versus interference screws", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 21, No. 3, (2005), 266-274. <https://doi.org/10.1016/j.arthro.2004.10.011>
50. Lenza, R. F. S., Jones, J. R., Vasconcelos, W. L., Hench, L. L., "In vitro release kinetics of proteins from bioactive foams", *Journal of Biomedical Materials Research Part A: An Official Journal of The Society for Biomaterials, The Japanese Society for Biomaterials, and The Australian Society for Biomaterials and the Korean Society for Biomaterials*, Vol. 67, No. 1, (2003), 121-129. <https://doi.org/10.1002/jbm.a.10042>
51. Nakafuku, C., Takehisa, S. Y., "Glass transition and mechanical properties of PLLA and PDLLA- PGA copolymer blends", *Journal of Applied Polymer Science*, Vol. 93, No. 5, (2004), 2164-2173. <https://doi.org/10.1002/app.20687>
52. Barber, F. A., "Poly-D, L-lactide interference screws for anterior cruciate ligament reconstruction", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 21, No. 7, (2005), 804-808. <https://doi.org/10.1016/j.arthro.2005.04.104>
53. Esmaeilzadeh, J., Hesaraki, S., Hadavi, S. M. M., Esfandeh, M., Ebrahimzadeh, M. H., "Microstructure and mechanical properties of biodegradable poly (D/L) lactic acid/polycaprolactone blends processed from the solvent-evaporation technique", *Materials Science and Engineering: C*, Vol. 71, (2017), 807-819. <https://doi.org/10.1016/j.msec.2016.10.070>
54. Esmaeilzadeh, J., Hesaraki, S., Hadavi, S. M. M., Ebrahimzadeh, M. H., Esfandeh, M., "Poly (D/L) lactide/polycaprolactone/bioactive glass nanocomposites materials for anterior cruciate ligament reconstruction screws: The effect of glass surface functionalization on mechanical properties and cell behaviors", *Materials Science and Engineering: C*, Vol. 77, (2017), 978-989. <https://doi.org/10.1016/j.msec.2017.03.134>
55. Martinek, V., Friederich, N. F., "Tibial and pretibial cyst formation after anterior cruciate ligament reconstruction with bioabsorbable interference screw fixation", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 15, No. 3, (1999), 317-320. [https://doi.org/10.1016/s0749-8063\(99\)70042-3](https://doi.org/10.1016/s0749-8063(99)70042-3)
56. Jagodzinski, M., Scheunemann, K., Knobloch, K., Albrecht, K., Krettek, C., Hurschler, C., Zeichen, J., "Tibial press-fit fixation of the hamstring tendons for ACL-reconstruction", *Knee Surgery, Sports Traumatology, Arthroscopy*, Vol. 14, No. 12, (2006), 1281-1287. <https://doi.org/10.1007/s00167-006-0105-y>
57. Lajtai, G., Schmiedhuber, G., Unger, F., Aitzetmüller, G., Klein, M., Noszian, I., Orthner, E., "Bone tunnel remodeling at the site of biodegradable interference screws used for anterior cruciate ligament reconstruction: 5-year follow-up", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 17, No. 6, (2001), 597-602. <https://doi.org/10.1053/jars.2001.21535>
58. Weimann, A., Zantop, T., Herbolt, M., Strobel, M., Petersen, W., "Initial fixation strength of a hybrid technique for femoral ACL graft fixation", *Knee Surgery, Sports Traumatology, Arthroscopy*, Vol. 14, No. 11, (2006), 1122-1129. <https://doi.org/10.1007/s00167-006-0159-x>
59. Pêgo, A. P., Grijpma, D. W., Feijen, J., "Enhanced mechanical properties of 1, 3-trimethylene carbonate polymers and networks", *Polymer*, Vol. 44, No. 21, (2003), 6495-6504. [https://doi.org/10.1016/s0032-3861\(03\)00668-2](https://doi.org/10.1016/s0032-3861(03)00668-2)
60. Farrar, D. F., Gillson, R. K., "Hydrolytic degradation of polyglyconate B: the relationship between degradation time, strength and molecular weight", *Biomaterials*, Vol. 23, No. 18, (2002), 3905-3912. [https://doi.org/10.1016/s0142-9612\(02\)00140-0](https://doi.org/10.1016/s0142-9612(02)00140-0)
61. Demirhan, M., Kilicoglu, O., Akpinar, S., Akman, S., Atalar, A. C., Göksan, M. A., "Time-dependent reduction in load to failure of wedge-type polyglyconate suture anchors", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 16, No. 4, (2000), 383-390. [https://doi.org/10.1016/s0749-8063\(00\)90083-5](https://doi.org/10.1016/s0749-8063(00)90083-5)

62. Nieminen, T., Rantala, I., Hiidenheimo, I., "Biodegradable plates and screws composed of L-lactide, D-lactide and trimethylenecarbonate: Properties during a 3-year follow-up", In *European Conference on Biomaterials*, Nantes, France, (2006).
63. Järvelä, T., Nurmi, J. T., Paakkala, A., Moissala, A. S., Kaikkonen, A., Järvinen, M., "Chapter 52 - Improving Biodegradable Interference Screw Properties by Combining Polymers", In *The Anterior Cruciate Ligament: Reconstruction and Basic Science*, Elsevier BV, (2008), 386–391. <http://doi.org/10.1016/b978-1-4160-3834-4.10052-6>
64. Barth, J., Akritopoulos, P., Gravelleau, N., Barthelemy, R., Toanen, C., Saffarini, M., "Efficacy of osteoconductive ceramics in bioresorbable screws for anterior cruciate ligament reconstruction: a prospective intrapatient comparative study", *Orthopaedic Journal of Sports Medicine*, Vol. 4, No. 5, (2016), 2325967116647724. <https://doi.org/10.1177/2325967116647724>
65. Lee, D. W., Lee, J. W., Kim, S. B., Park, J. H., Chung, K. S., Ha, J. K., Kim, J. G., Kim, W. J., "Comparison of poly-L-lactic acid and poly-L-lactic acid/hydroxyapatite bioabsorbable screws for tibial fixation in ACL reconstruction: clinical and magnetic resonance imaging results", *Clinics in Orthopedic Surgery*, Vol. 9, No. 3, (2017), 270-279. <https://doi.org/10.4055/cios.2017.9.3.270>
66. Hunt, J. A., Callaghan, J. T., "Polymer-hydroxyapatite composite versus polymer interference screws in anterior cruciate ligament reconstruction in a large animal model", *Knee Surgery, Sports Traumatology, Arthroscopy*, Vol. 16, No. 7, (2008), 655-660. <https://doi.org/10.1007/s00167-008-0528-8>
67. Barber, F. A., Dockery, W. D., "Long-term absorption of poly-L-lactic acid interference screws", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 22, No. 8, (2006), 820-826. <https://doi.org/10.1016/j.arthro.2006.04.096>
68. Barber, F. A., Dockery, W. D., "Long-Term Degradation of Self-Reinforced Poly-Levo (96%)/Dextro (4%)–Lactide/ β -Tricalcium Phosphate Biocomposite Interference Screws", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 32, No. 4, (2016), 608-614. <https://doi.org/10.1016/j.arthro.2015.08.037>
69. Ntgiopoulos, P. G., Demey, G., Tavernier, T., Dejour, D., "Comparison of resorption and remodeling of bioabsorbable interference screws in anterior cruciate ligament reconstruction", *International Orthopaedics*, Vol. 39, No. 4, (2015), 697-706. <https://doi.org/10.1007/s00264-014-2530-8>
70. Barber, F. A., Dockery, W. D., "Biocomposite Interference Screws in Anterior Cruciate Ligament Reconstruction: Osteoconductivity and Degradation", *Arthroscopy, Sports Medicine, and Rehabilitation*, Vol. 2, No. 2, (2020), e53–e58. <http://doi.org/10.1016/j.asmr.2019.10.001>
71. Walsh, W. R., Cotton, N. J., Stephens, P., Brunelle, J. E., Langdown, A., Auld, J., Vizesi, F., Bruce, W., "Comparison of poly-L-lactide and polylactide carbonate interference screws in an ovine anterior cruciate ligament reconstruction model", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 23, No. 7, (2007), 757-765. <https://doi.org/10.1016/j.arthro.2007.01.030>
72. Agrawal, C. M., Athanasiou, K. A., "Technique to control pH in vicinity of biodegrading PLA- PGA implants", *Journal of biomedical materials research*, Vol. 38, No. 2, (1997), 105-114. [https://doi.org/10.1002/\(sici\)1097-4636\(199722\)38:2%3C105::aid-jbm4%3E3.0.co;2-u](https://doi.org/10.1002/(sici)1097-4636(199722)38:2%3C105::aid-jbm4%3E3.0.co;2-u)
73. Cooper, J. J., Mackie, A. T., "In vitro evaluation of a range of bioabsorbable composite interference screws designed for anterior cruciate ligament reconstruction", In *54th Annual Meeting of the Orthopaedic Research Society, San Francisco, CA*, February 2008, (2008). <https://www.ors.org/Transactions/54/1278.pdf>
74. Aunoble, S., Clément, D., Frayssinet, P., Harmand, M. F., Le Huec, J. C., "Biological performance of a new β -TCP/PLLA composite material for applications in spine surgery: In vitro and in vivo studies", *Journal of Biomedical Materials Research Part A: An Official Journal of The Society for Biomaterials, The Japanese Society for Biomaterials, and The Australian Society for Biomaterials and the Korean Society for Biomaterials*, Vol. 78, No. 2, (2006), 416-422. <https://doi.org/10.1002/jbm.a.30749>
75. Purcell, D. B., Rudzki, J. R., Wright, R. W., "Bioabsorbable interference screws in ACL reconstruction", *Operative Techniques in Sports Medicine*, Vol. 12, No. 3, (2004), 180-187. <https://doi.org/10.1053/j.otsm.2004.07.014>
76. Pigni, M., Leardi, G., Battistella, F., Bernasconi, S., "Hamstring anterior cruciate ligament reconstruction in skiers: tibial fixation with bioabsorbable or not bioabsorbable system", In *International Congress*, (2006).
77. Poandl, T., Trenka-Benthin, S., Azri-Meehan, S., Contiliano, J., Li, Y., Yuan, J., TenHuisen, K., Dooley, J., Zimmerman, M., "A new faster-absorbing biocomposite material: Long-term in-vivo tissue reaction and absorption", E-poster presented at: *Spring Arthroscopy Association of North America (AANA) Meeting, Vancouver, Canada*, May 2005, (2005), E-09. <http://prod.mitek.depuj.edgesuite.net/PDFsforWebsite/900858.pdf>
78. Siebold, R., "Observations on Bone Tunnel Enlargement After Double-Bundle Anterior Cruciate Ligament Reconstruction", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 23, No. 3, (2007), 291–298. <http://doi.org/10.1016/j.arthro.2007.01.006>
79. LeGeros, R. Z., LeGeros, J. P., "Dense hydroxyapatite", In *An Introduction to Bioceramics*, (1993), 139-180. https://doi.org/10.1142/9789814317351_0009
80. Bailey, C. A., Kuiper, J. H., Kelly, C. P., "Biomechanical evaluation of a new composite bioresorbable screw", *Journal of Hand Surgery*, Vol. 31, No. 2, (2006), 208-212. <https://doi.org/10.1016/j.jhsb.2005.10.015>
81. Tecklenburg, K., Burkart, P., Hoser, C., Rieger, M., Fink, C., "Prospective evaluation of patellar tendon graft fixation in anterior cruciate ligament reconstruction comparing composite bioabsorbable and allograft interference screws", *Arthroscopy: The Journal of Arthroscopic & Related Surgery*, Vol. 22, No. 9, (2006), 993-999. <https://doi.org/10.1016/j.arthro.2006.05.010>
82. Baums, M. H., Zelle, B. A., Schultz, W., Ernstberger, T., Klinger, H. M., "Intraarticular migration of a broken biodegradable interference screw after anterior cruciate ligament reconstruction", *Knee Surgery, Sports Traumatology, Arthroscopy*, Vol. 14, No. 9, (2006), 865-868. <https://doi.org/10.1007/s00167-006-0049-2>
83. Krappel, F. A., Bauer, E., Harland, U., "The migration of a BioScrew® as a differential diagnosis of knee pain, locking after ACL reconstruction: a report of two cases", *Archives of Orthopaedic and Trauma Surgery*, Vol. 126, No. 9, (2006), 615-620. <https://doi.org/10.1007/s00402-006-0101-1>
84. Wang, J., Wu, Y., Li, H., Liu, Y., Bai, X., Chau, W., Zheng, Y., Qin, L., "Magnesium alloy based interference screw developed for ACL reconstruction attenuates peri-tunnel bone loss in rabbits", *Biomaterials*, Vol. 157, (2018), 86-97. <https://doi.org/10.1016/j.biomaterials.2017.12.007>
85. Song, B., Li, W., Chen, Z., Fu, G., Li, C., Liu, W., Li, Y., Qin, L., Ding, Y., "Biomechanical comparison of pure magnesium interference screw and polylactic acid polymer interference screw in anterior cruciate ligament reconstruction—A cadaveric experimental study", *Journal of Orthopaedic Translation*, Vol. 8, (2017), 32-39. <https://doi.org/10.1016/j.jot.2016.09.001>
86. Agarwal, S., Curtin, J., Duffy, B., Jaiswal, S., "Biodegradable magnesium alloys for orthopaedic applications: A review on corrosion, biocompatibility and surface modifications", *Materials Science and Engineering: C*, Vol. 68, (2016), 948-963. <https://doi.org/10.1016/j.msec.2016.06.020>

87. Zheng Y. F., Gu, X. N., Witte, F., "Biodegradable metals", *Materials Science and Engineering: R: Reports*, Vol. 77, (2014), 1–34. <http://doi.org/10.1016/j.msere.2014.01.001>
88. Li, N., Zheng, Y., "Novel magnesium alloys developed for biomedical application: a review", *Journal of Materials Science & Technology*, Vol. 29, No. 6, (2013), 489-502. <https://doi.org/10.1016/j.jmst.2013.02.005>
89. Cheng, P., Han, P., Zhao, C., Zhang, S., Zhang, X., Chai, Y., "Magnesium inference screw supports early graft incorporation with inhibition of graft degradation in anterior cruciate ligament reconstruction", *Scientific Reports*, Vol. 6, (2016), p.26434. <https://doi.org/10.1038/srep26434>
90. Yao, Y., Wang, L., Li, J., Tian, S., Zhang, M., Fan, Y., "A novel auxetic structure based bone screw design: Tensile mechanical characterization and pullout fixation strength evaluation", *Materials & Design*, Vol. 188, (2020), 108424. <https://doi.org/10.1016/j.matdes.2019.108424>
91. Butler, D. L., "Anterior cruciate ligament: Its normal response and replacement", *Journal of Orthopaedic Research*, Vol. 7, No. 6, (1989), 910-921. <https://doi.org/10.1002/jor.1100070618>
92. Rodeo, S. A., Arnoczky, S. P., Torzilli, P. A., Hidaka, C., Warren, R. F., "Tendon-healing in a bone tunnel. A biomechanical and histological study in the dog", *The Journal of bone and joint surgery. American volume*, Vol. 75, No. 12, (1993), 1795-1803. <https://doi.org/10.2106/00004623-199312000-00009>
93. Beevers, D. J., "Metal vs bioabsorbable interference screws: initial fixation", *Proceedings of the Institution of Mechanical Engineers, Part H: Journal of Engineering in Medicine*, Vol. 217 No. 1, (2003), 59-75. <https://doi.org/10.1243/095441103762597746>
94. Roesler, C. R. M., Salmoria, G. V., Moré, A. D. O., Vassoler, J. M., Fancello, E. A., "Torsion test method for mechanical characterization of PLDLA 70/30 ACL interference screws", *Polymer Testing*, Vol. 34, (2014), 34-41. <https://doi.org/10.1016/j.polymertesting.2013.12.005>
95. Nyland, J., Krupp, R., Greene, J., Bowles, R., Burden, R., Caborn, D. N., "In situ comparison of varying composite tibial tunnel interference screws used for ACL soft tissue graft fixation", *The Knee*, Vol. 22, No. 6, (2015), 554-558. <https://doi.org/10.1016/j.knee.2015.03.009>
96. Schumacher, T. C., Tushtev, K., Wagner, U., Becker, C., große Holthaus, M., Hein, S. B., Haack, J., Heiss, C., Engelhardt, M., El Khassawna, T., Rezwan, K., "A novel, hydroxyapatite-based screw-like device for anterior cruciate ligament (ACL) reconstructions", *The Knee*, Vol. 24, No. 5, (2017), 933-939. <https://doi.org/10.1016/j.knee.2017.07.005>
97. Resende, J. L., Faria, M. T. C., Las Casas, E. B., Oliveira, E. A., Gomes, P. D. T. V., "Mechanical properties characterization of knee cruciate ligaments through tensile tests", In *Proceedings of the 18th International Congress of Mechanical Engineering (COBEM 2005), Ouro Preto-MG, Brazil*, 6-11 November 2005, (2005), 1-7.
98. "Arthrex BioComposite interference screws for ACL and PCL reconstruction", LA1-0150-EN_E, Naples, FL, (2018).
99. Kousa, P., Järvinen, T. L., Kannus, P., Järvinen, M., "Initial fixation strength of bioabsorbable and titanium interference screws in anterior cruciate ligament reconstruction: biomechanical evaluation by single cycle and cyclic loading", *The American Journal of Sports Medicine*, Vol. 29, No. 4, (2001), 420-425. <https://doi.org/10.1177/03635465010290040601>
100. Moré, A. D. O., Pizzolatti, A. L. A., Fancello, E. A., Salmoria, G.V., Roesler, C. R. D. M., "Graft tendon slippage with metallic and bioabsorbable interference screws under cyclic load: a biomechanical study in a porcine model", *Research on Biomedical Engineering*, Vol. 31, No. 1, (2015), 56-61. <https://doi.org/10.1590/2446-4740.0652>